



Topcon Aladdin Biometer

Patient : TOPCON DEMO

Surgeon : Surgeon Generic

Patient ID :

Exam Date : 02/10/2015 - 17:55
(mm/dd/yyyy)

Date Of Birth : 01/01/1950
(mm/dd/yyyy)

Dynamic Pupillometry

OD

Diameter (mm)

| Min | Max |
|------|------|
| 3.48 | 4.98 |



Center (mm)

| Mean | Std Dev |
|----------|---------|
| x= -0.27 | 0.07 |
| y= 0.02 | |

OS

Diameter (mm)



| Min | Max |
|------|------|
| 3.27 | 4.78 |



Center (mm)

| Mean | Std Dev |
|----------|---------|
| x= 0.25 | 0.08 |
| y= -0.04 | |

Latency

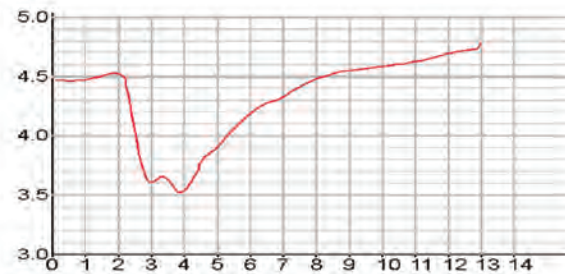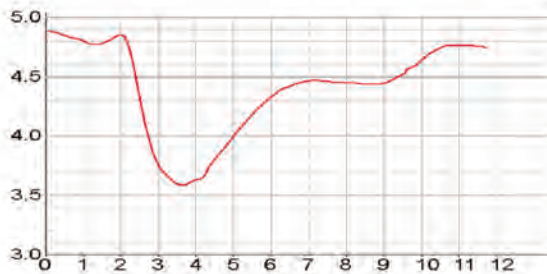

Static Pupillometry

Diameter (mm)

| | Mesopic | Photopic |
|---------|---------|----------|
| Mean | 4.57 | 3.80 |
| Std Dev | 0.09 | 0.09 |

Center (mm)

| | Mesopic | Photopic |
|---|---------|----------|
| X | -0.33 | -0.27 |
| Y | 0.04 | -0.01 |



Diameter (mm)

| | Mesopic | Photopic |
|---------|---------|----------|
| Mean | 4.60 | 3.71 |
| Std Dev | 0.09 | 0.10 |

Center (mm)

| | Mesopic | Photopic |
|---|---------|----------|
| X | 0.25 | 0.21 |
| Y | -0.15 | -0.09 |

